



Point Of Use Preparation
Point Of Use
Instrument Prep
Instrument Pre Soak
Point Of Use

Medisafe

Distal Duck Tip Soaker


Keeping complex instruments moist after use



- Retains moisture around distal tips for easy cleaning - enzyme concentrate soaks distal tip
- Recommended by leading manufacturer's IFU's for keeping instruments moist between point of use (OR) and reprocessing (CSSD).
- Safe - Duck vial is also instrument / distal tip protector
- Suitable for all instruments*
- 4 Active Enzymes - works at room temperature
- pH Neutral - non-corrosive
- Safe, quick and convenient use
- No more pre-soaking in CSSD

*Check with instrument manufacturer's IFU's

As recommended by leading surgical instrument manufacturers, keeping instruments moist immediately after use is a critical first step to effective "point of use preparation", safe transport and subsequent decontamination.

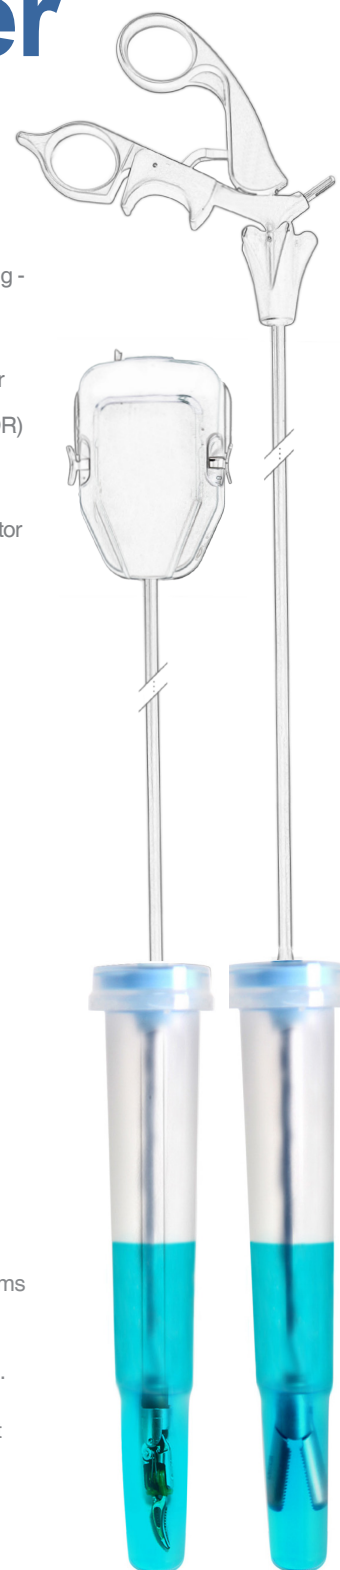

6.4 Containment (ST79:2010/A3:2012) Immediately after use, items should be kept moist.

Rationale: Containment minimizes the possibility of airborne or contact spread of microorganisms. Keeping items moist prevents soil from drying on device surfaces and facilitates the decontamination process.

7.3 Presoaking Presoaking with a specialized product (e.g. an enzymatic solution) is generally recommended.

Presoaking should begin as soon as possible after an instrument is used.

Rationale: Presoaking instruments moistens and loosens the soil, thus making the cleaning step more efficient

DOH, CFPP 01-01, Page 20 "Prions are hydrophobic proteins. The attachment of hydrophobic proteins to surfaces becomes less reversible if they are allowed to dry fully onto a surface. Keeping the environment around soiled instruments at or near saturation humidities (moist) prevents full attachment of hydrophobic proteins such that they are more efficiently removed by cleaning."


EN ISO 15883-2: 2009 "The efficacy of disinfection can be impaired if soil removal is incomplete before the start of the disinfection process. Users should be aware that some medical devices might require pre-treatment"

Order details:

Distal Tip Soaker

M20413

250 Vials per box





Point Of Use Preparation
Point Of Use
Instrument Prep
Instrument Pre Soak
Point Of Use


Distal Duck Tip Soaker

Keeping complex instruments moist after use




Name:	Distal Duck Tip Soaker
Classification:	CE marked Class 1
Ingredients	pH neutral aqueous solution of proteases, lipase and amylase enzymes with corrosion inhibitor, preservatives and surfactants
Storage condition	between 2°C and 38°C (35.6°F - 100.40°F)
pH	7.5-8.2
Shelf life	Up to 2 years
Packaging:	250 vials per box

Instructions For Use Distal Duck Tip Soaker

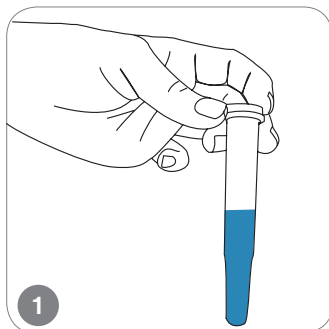


1

Ready

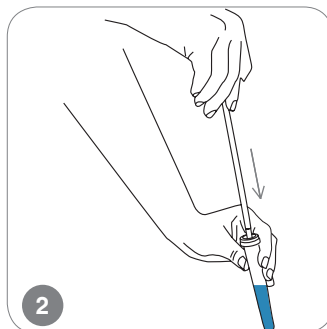

2

Insert

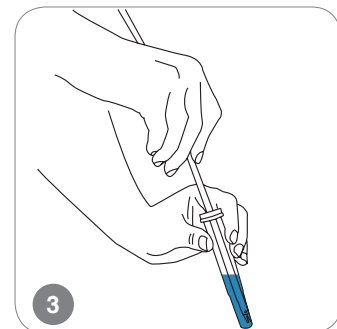


3

Soak




4

Transport

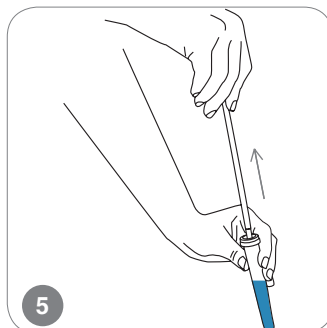

5

Remove

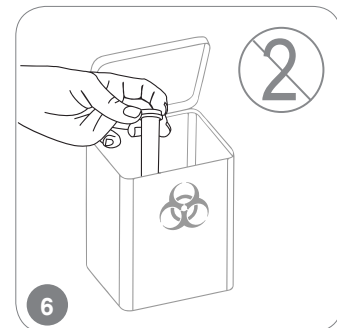

6

Discard